




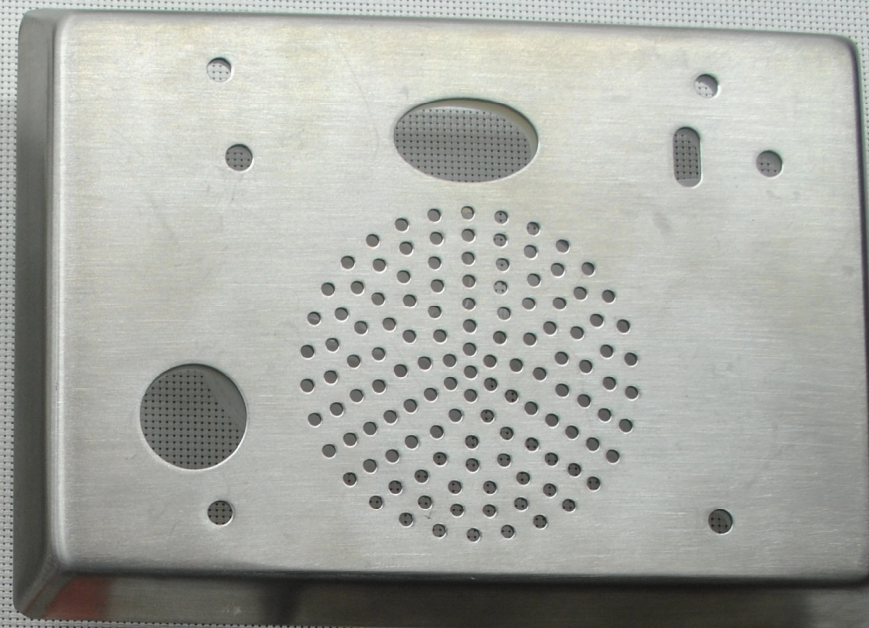

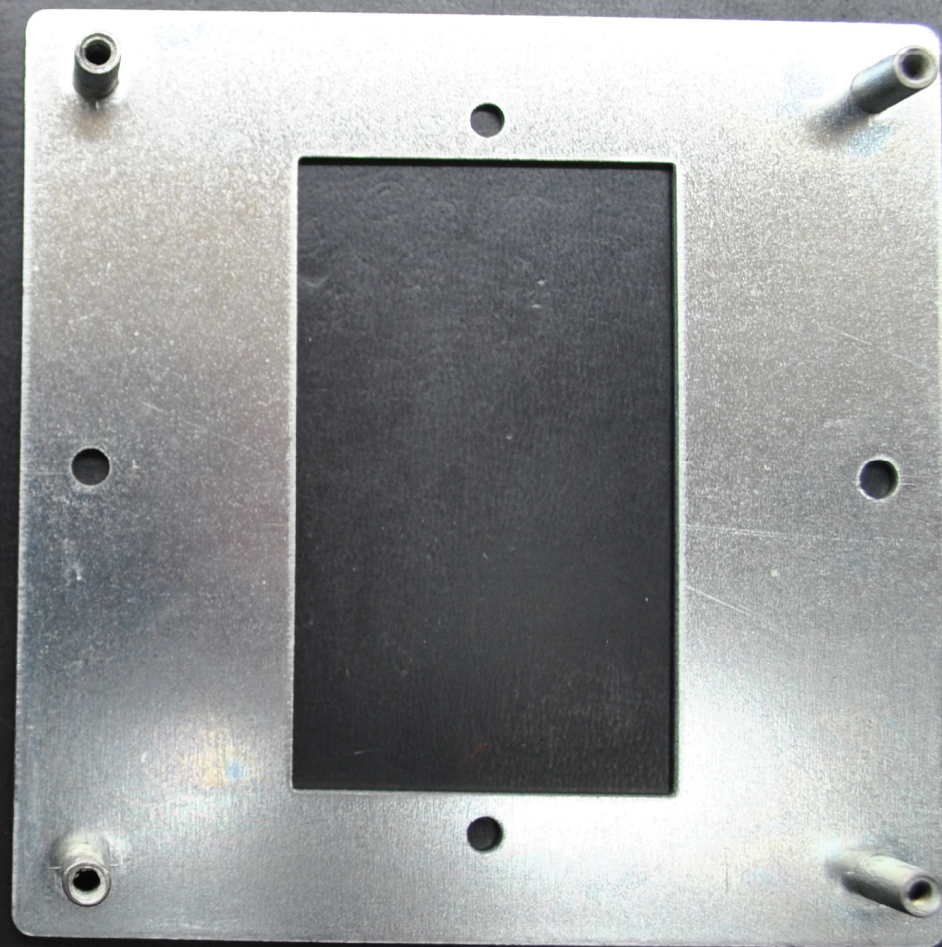


Required Room Equipment:

- 2-353101 Staff Station
- 2-R5HSSCP-1
- 1-R5KLS-4
- 1-352010 Domelight
- 3-354100- Input Module
- 2-R5WPPB Water Resistant Call Switch
- 1-350005 M Net Divider

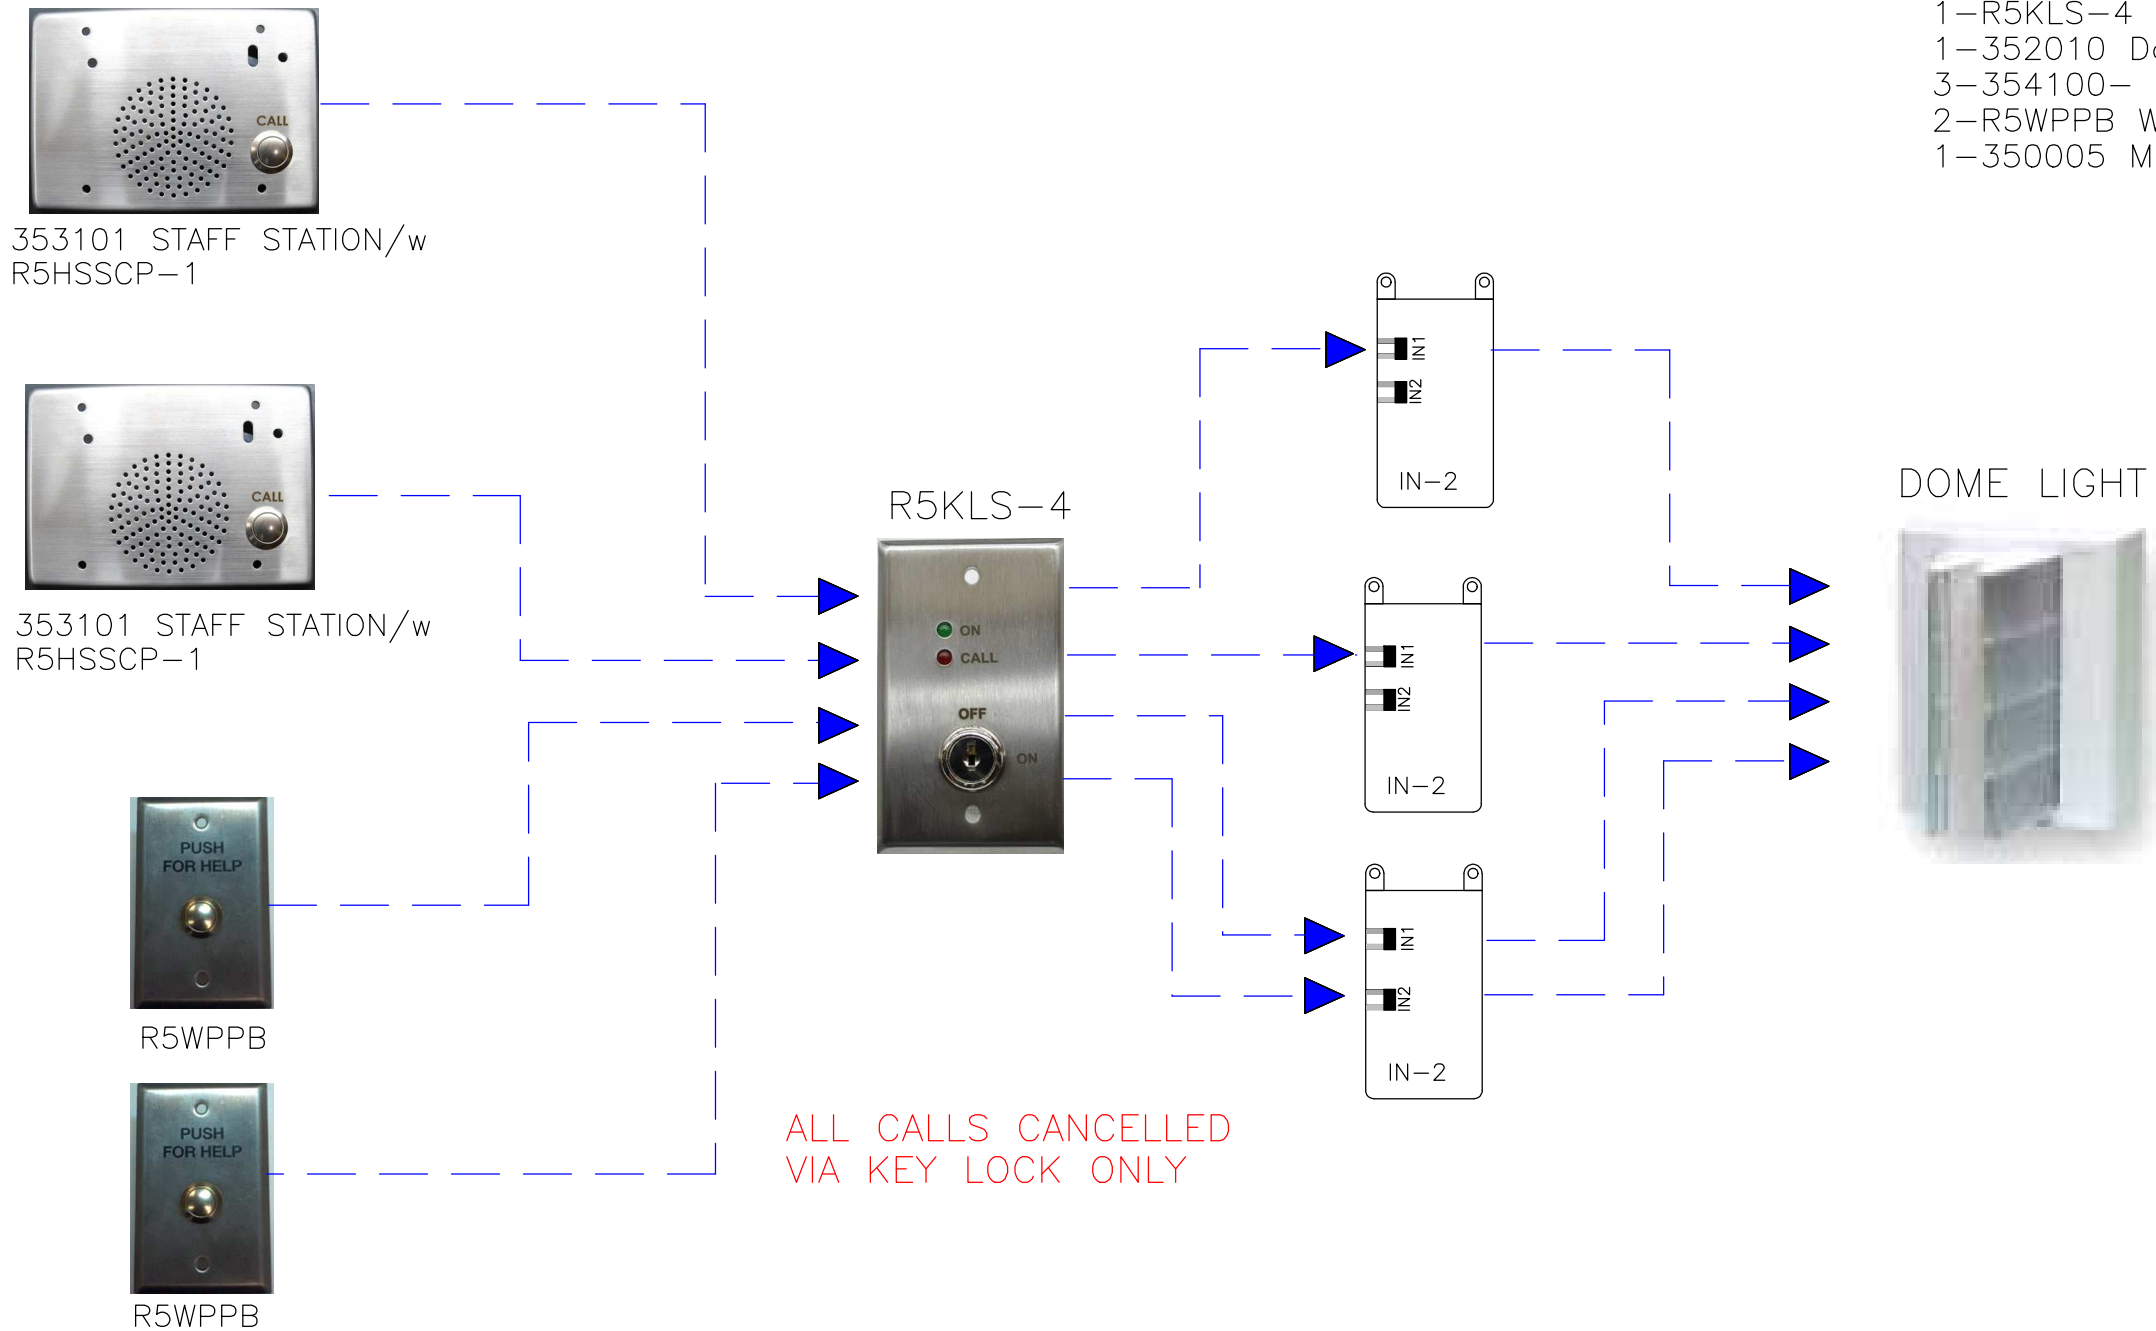

R5 High Security Key Lock Solution Option 1

- Required Room Equipment:
- 3-353101 Staff Station
 - 3-R5HSSCP-1
 - 1-R5KLS-4
 - 1-352010 Domelight
 - 3-354100- Input Module
 - 1- R5WPPB Water Resistant Call Switch
 - 2-350005 M Net Divider

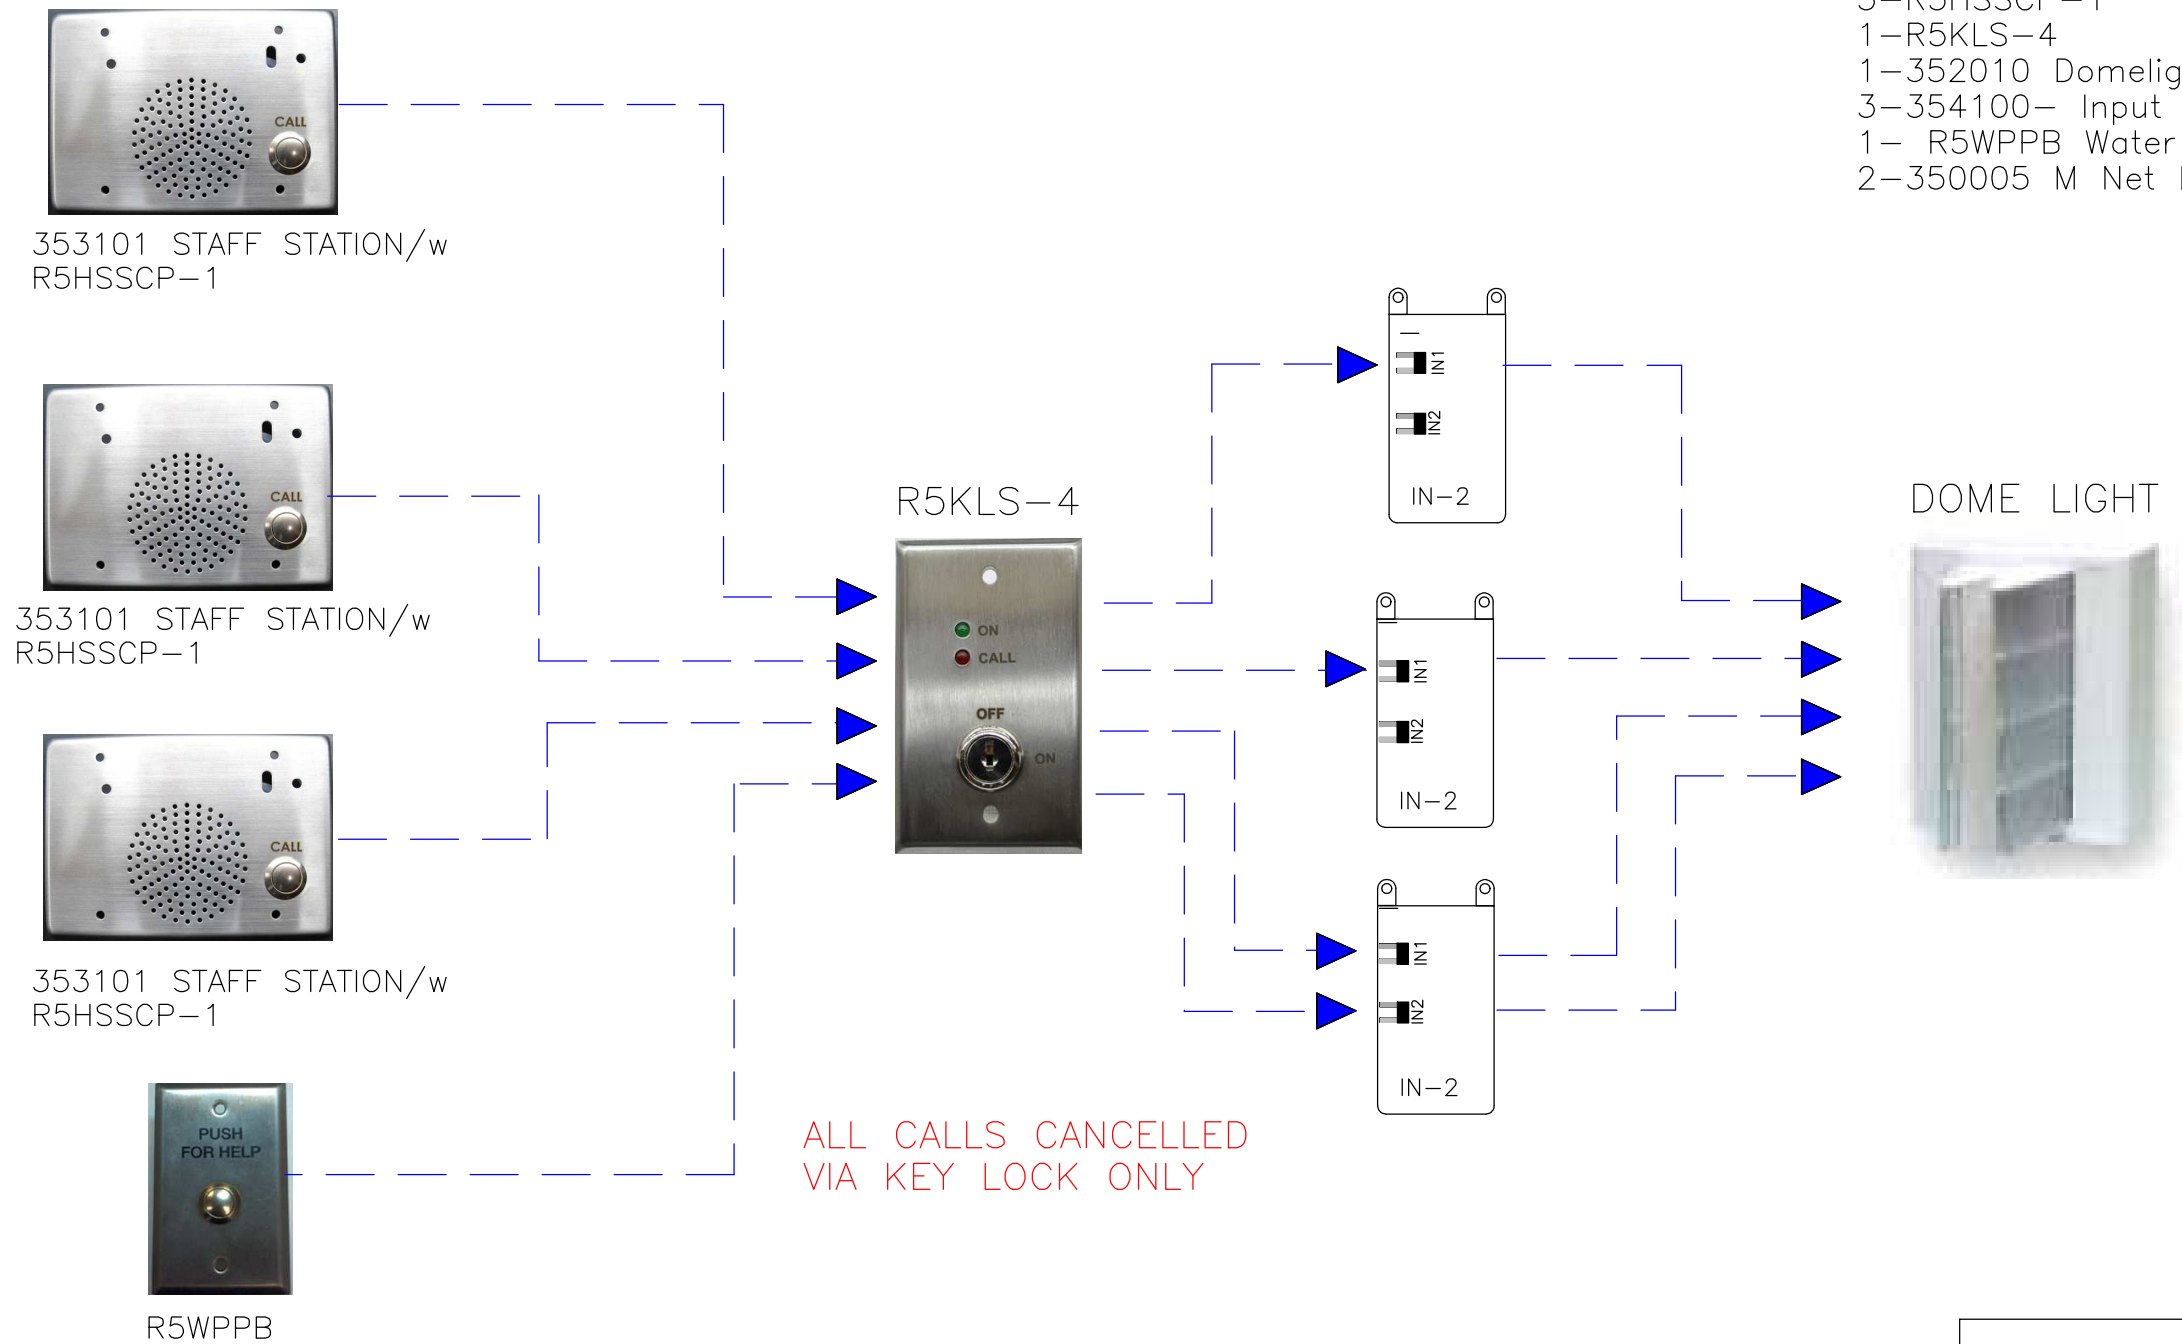


BLUE LINE REPRESENTS
CALL PATHWAY


R5 High Security Key Lock Solution Option 1A

Required Room Equipment:

- 2-353101 Staff Station
- 2-R5HSSCP-1
- 1-R5KLS-4
- 1-352021 Domeless Controller
- 3-354100-Input Module
- 1-354102 Relay Output Module
- 2-R5WPPB Water Resistant Call Switch
- 2-350005 M Net Divider
- 1- CLS-103 Dome Light

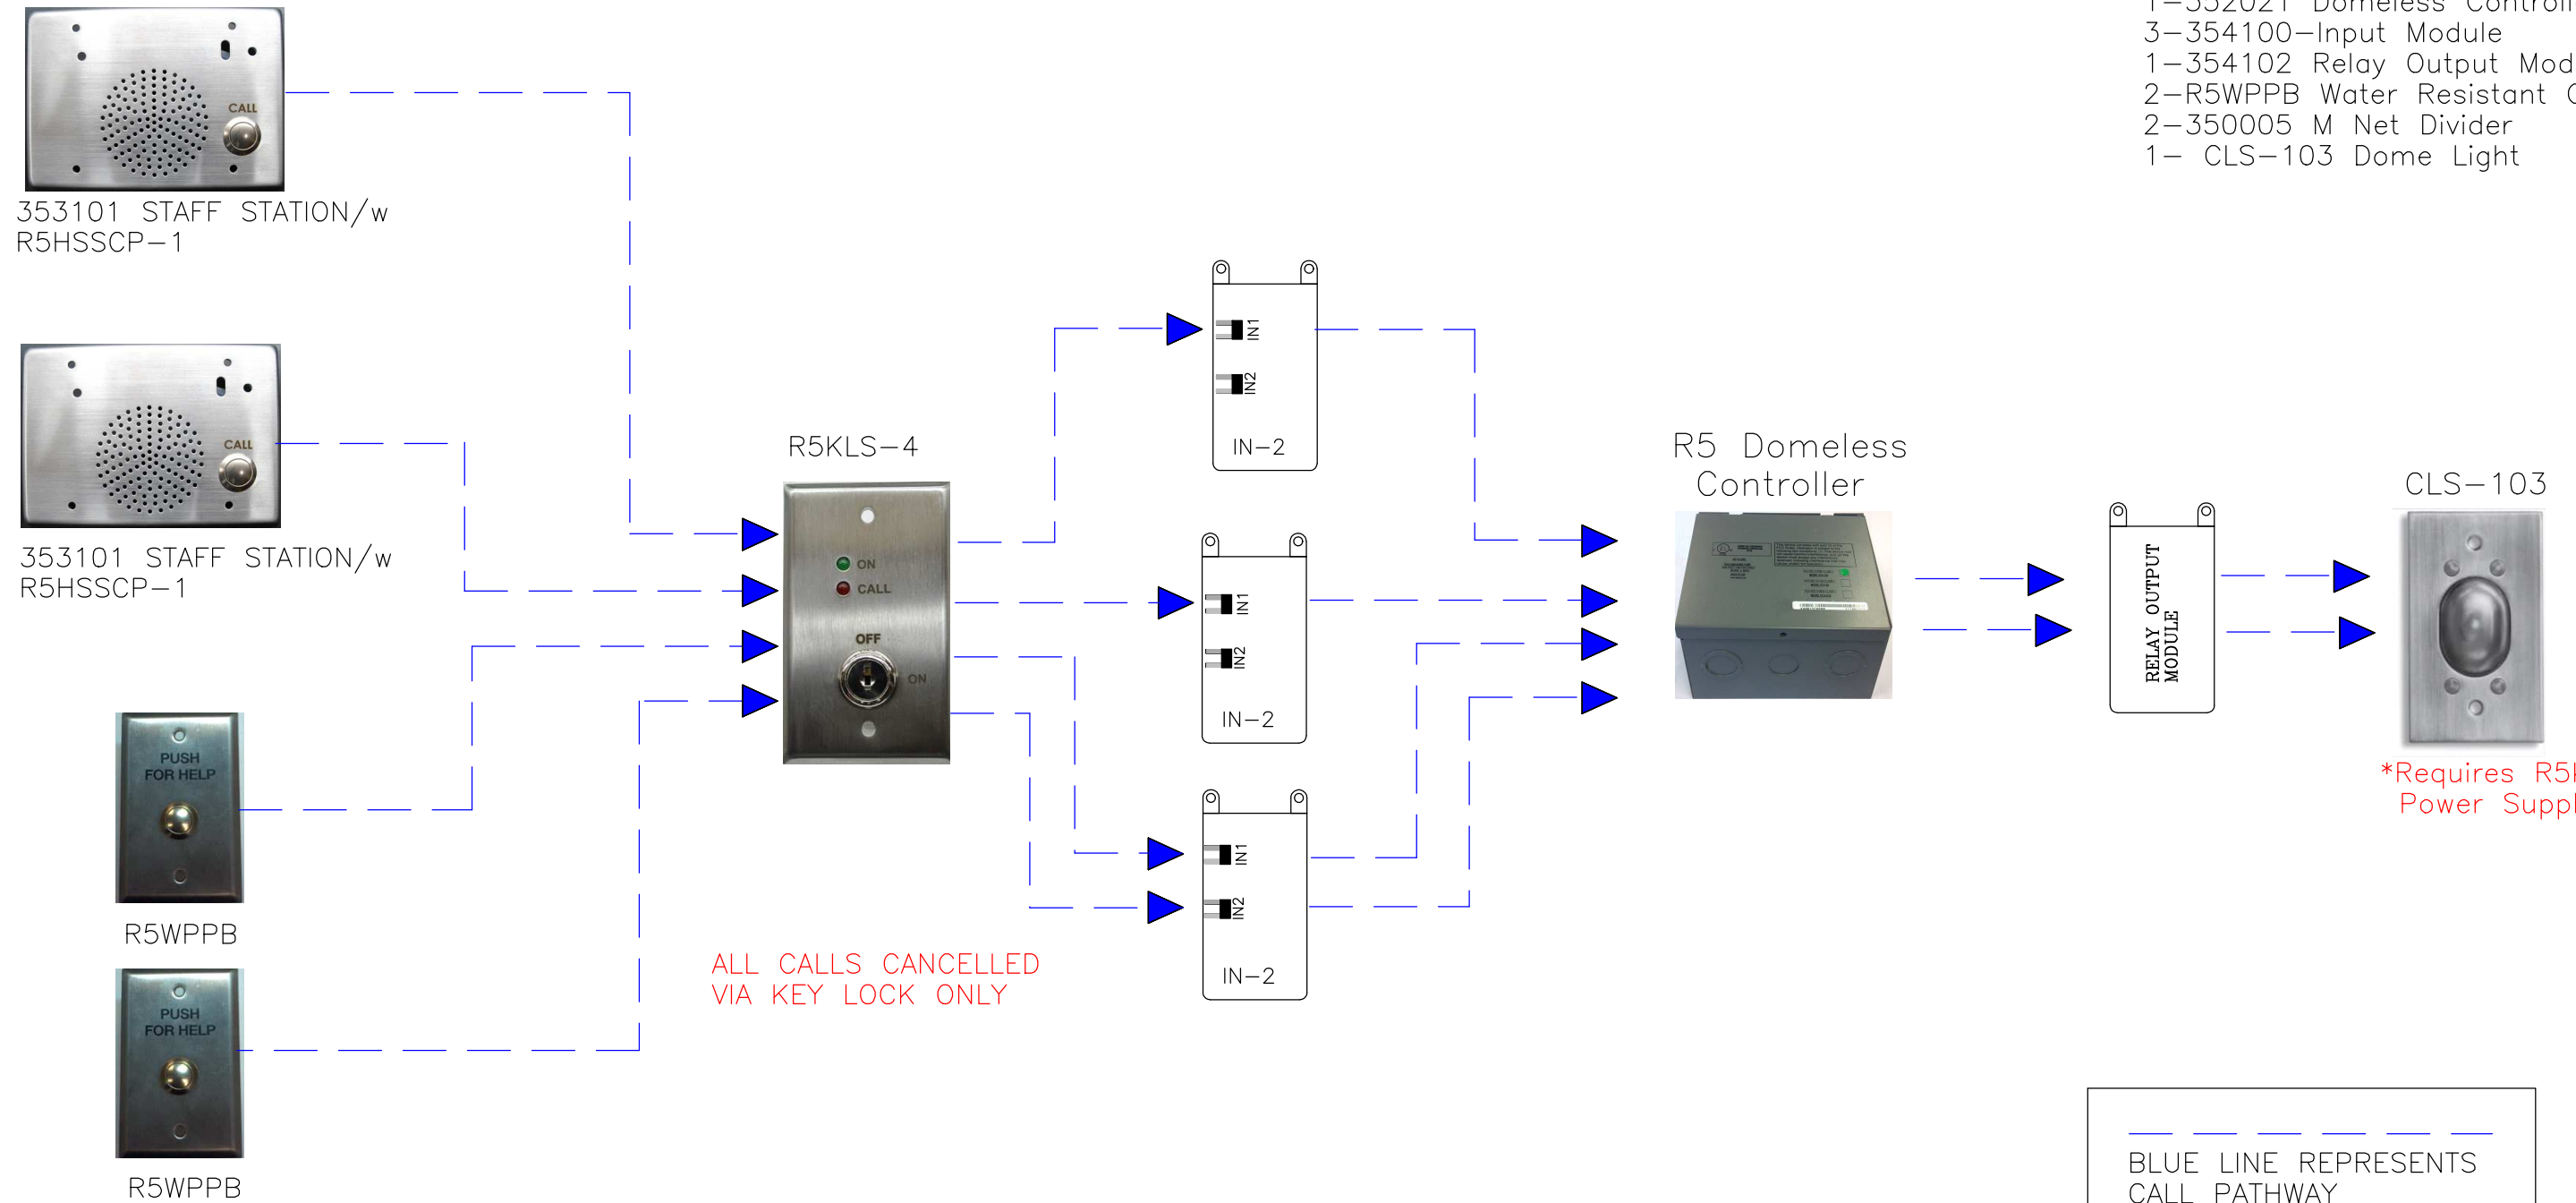


R5 High Security Key Lock Solution Option 2

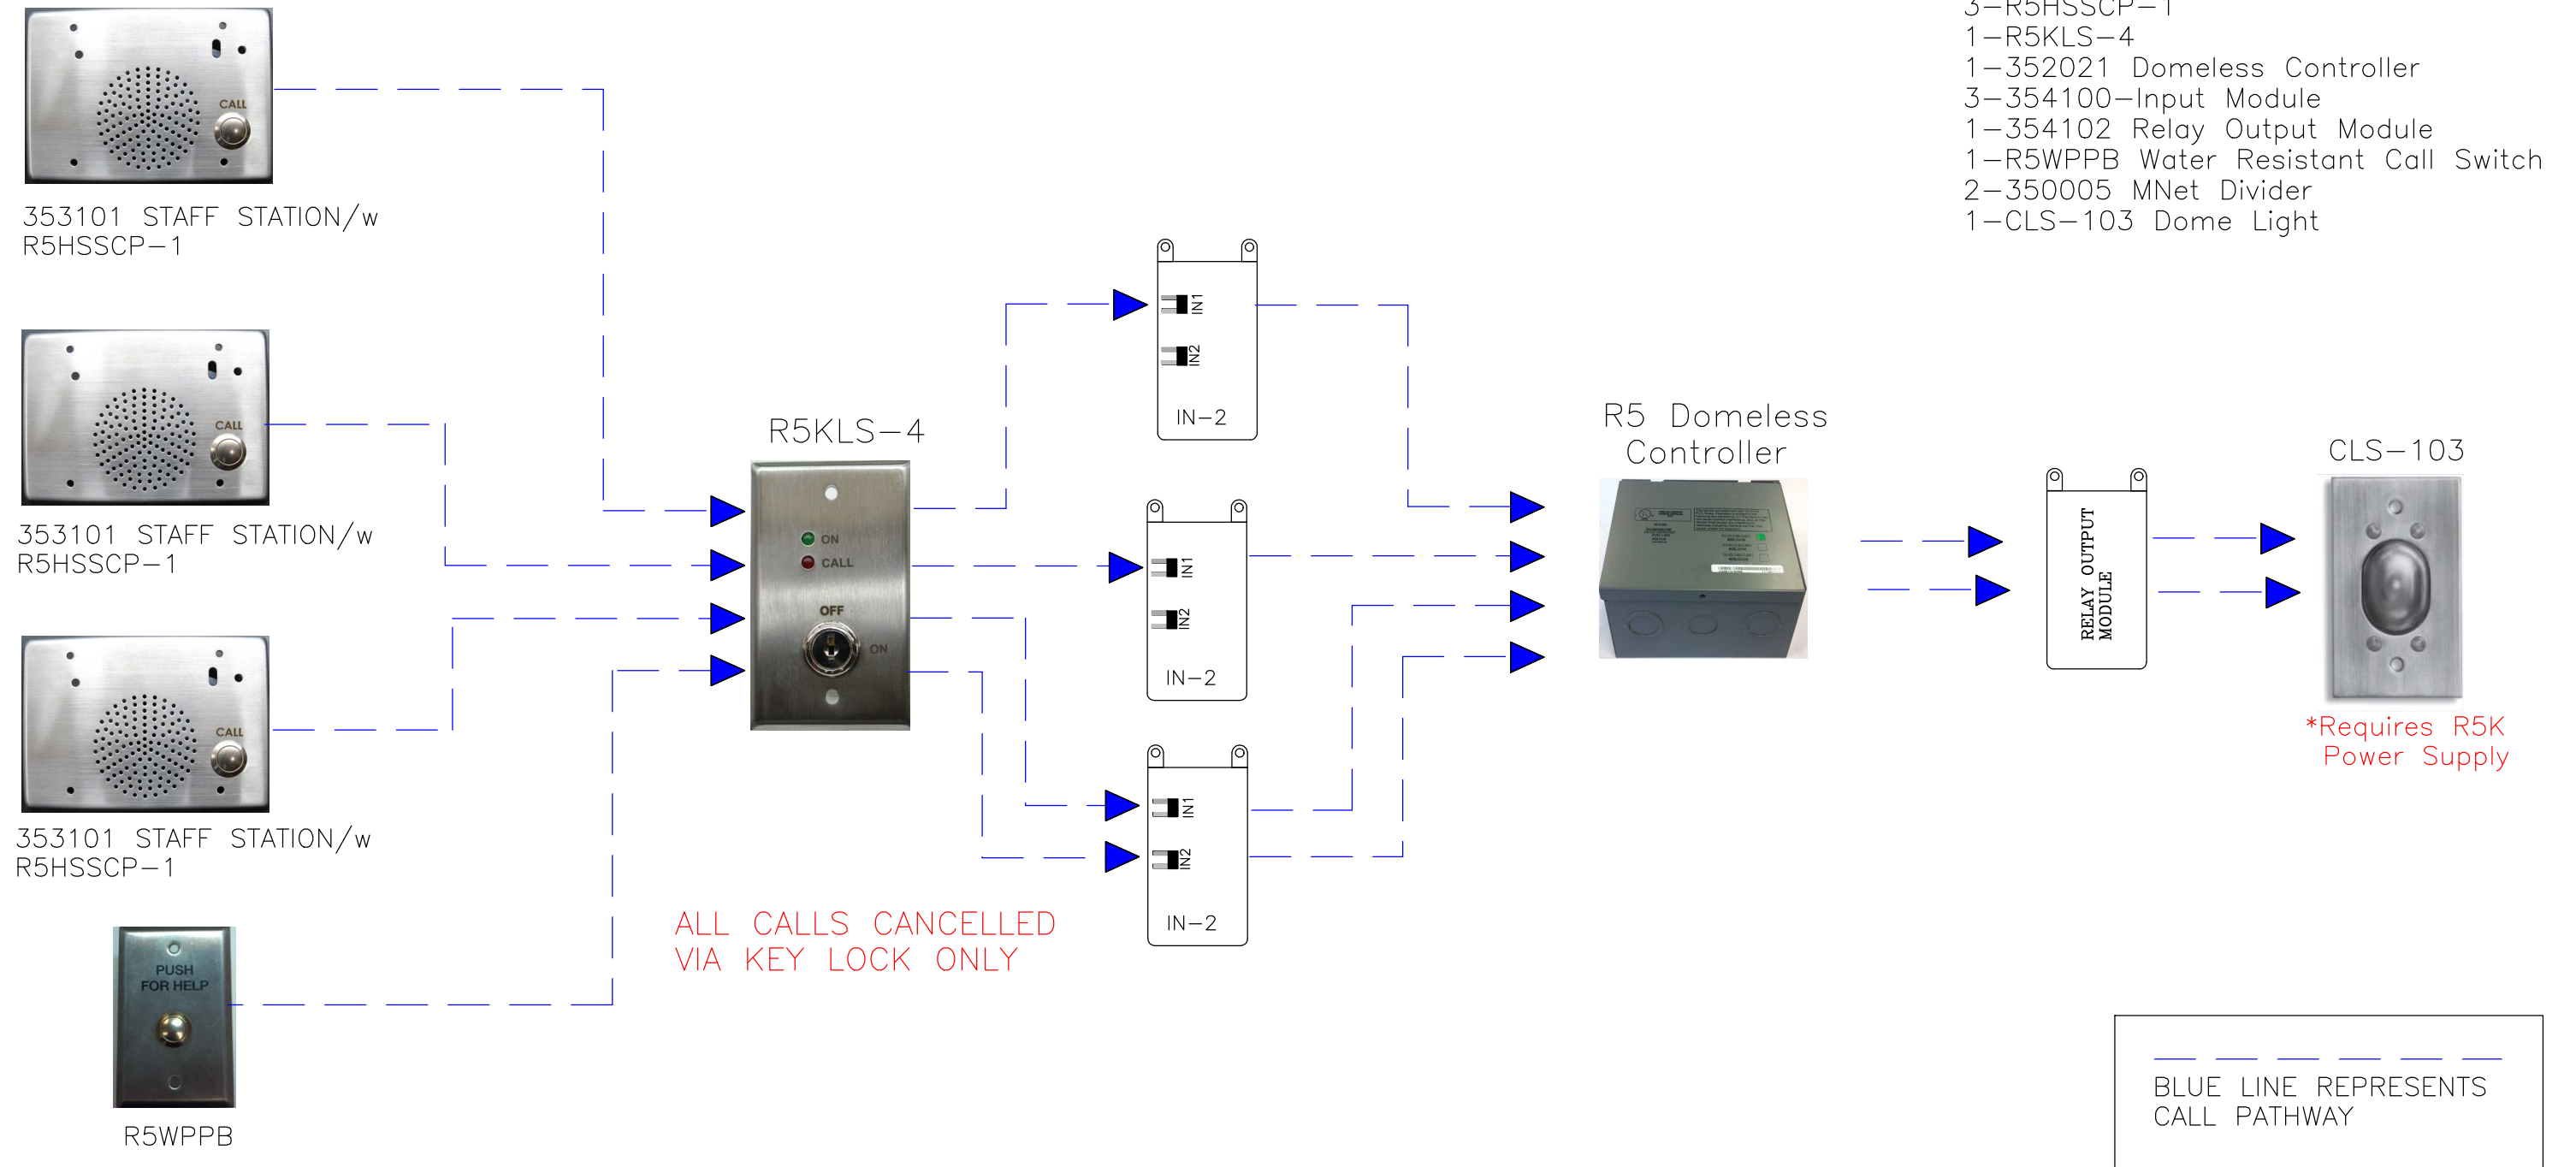

Required Room Equipment:


- 2-353101 Staff Station
- 2-R5HSSCP-2
- 1-352010 Domelight
- 1-354100- Input Module (min)
- 1-R5WPPB Water Resistant Call Switch
- 1-350005 M Net Divider
- 1-354012 (PBS1) Order QP1804 Button
- 1-354012 Staff Assist Station
- 1-R5HSPBCP

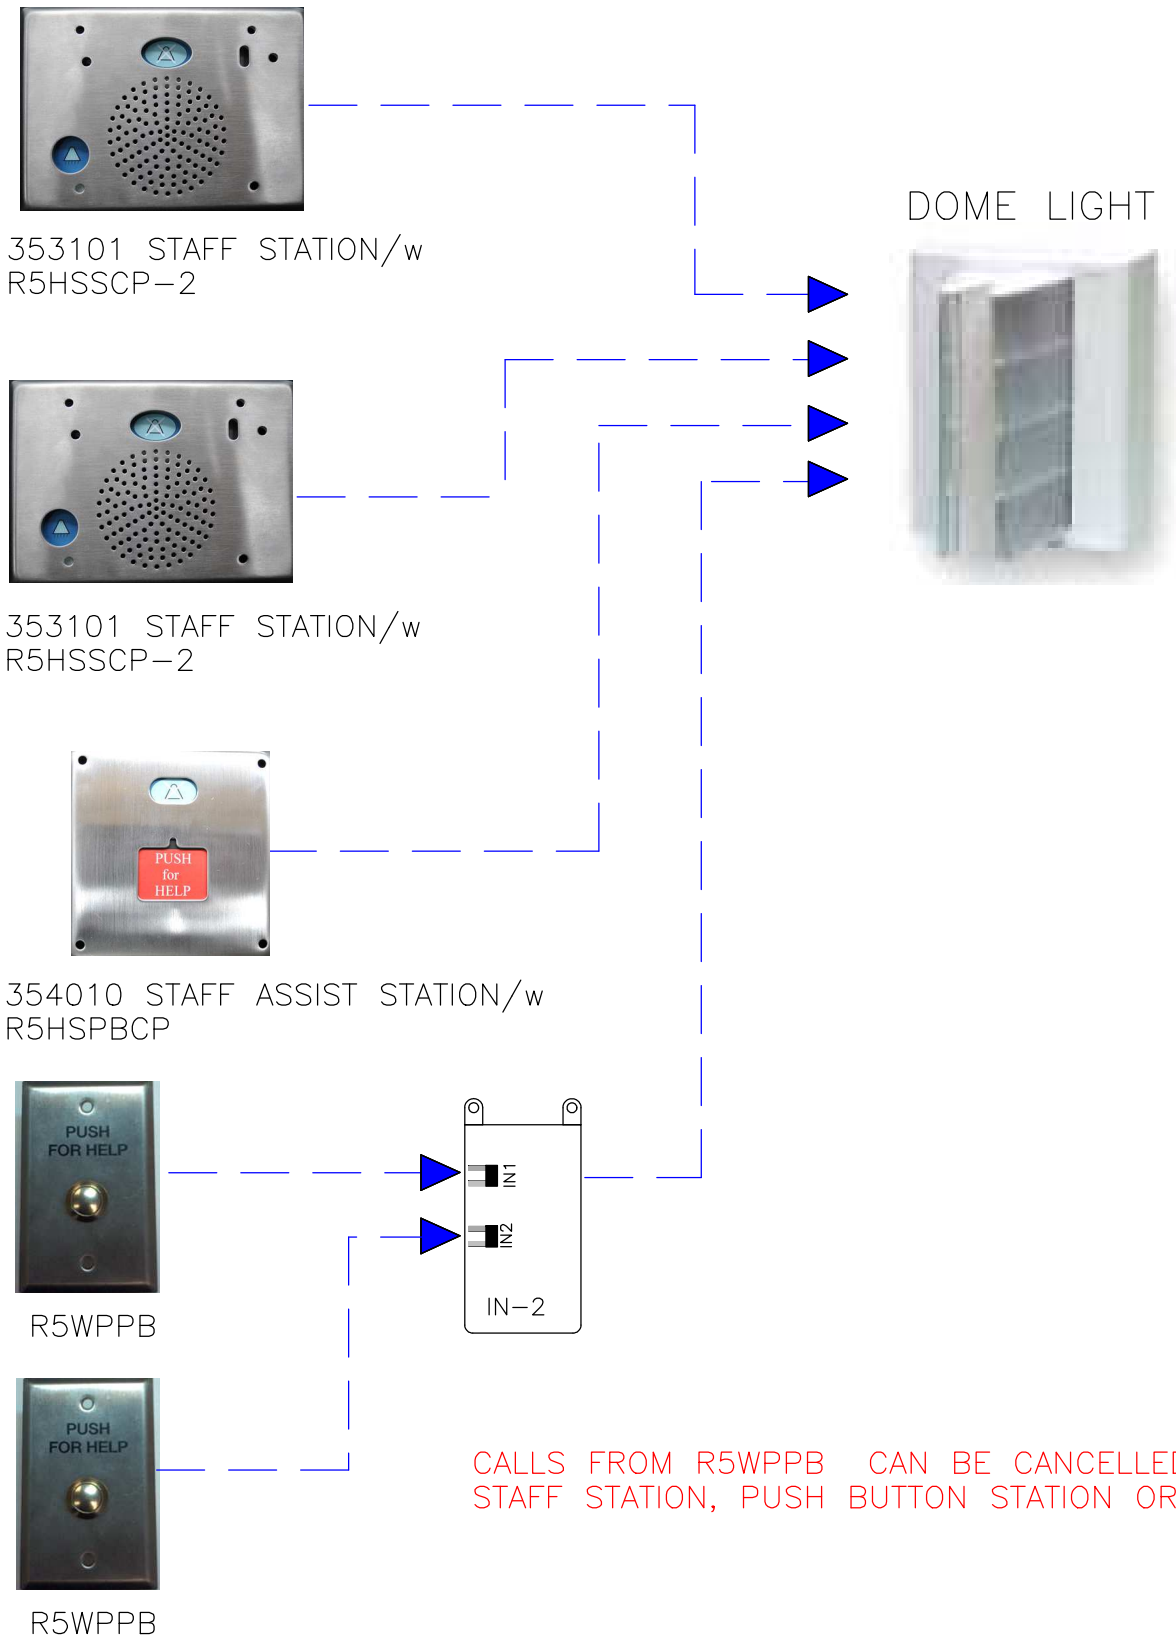

BLUE LINE REPRESENTS
CALL PATHWAY

R5 High Security Key Lock Solution Option 3


- Required Room Equipment:
- 2-353101 Staff Station
 - 2-R5HSSCP-2
 - 1-352010 Domelight
 - 1-354100- Input Module (min)
 - 1-R5WPPB Water Resistant Call Switch
 - 1-350005 M Net Divider
 - 1-354012 (PBS1) Order QP1804 Button
 - 1-354012 Staff Assist Station
 - 1-R5HSPBCP

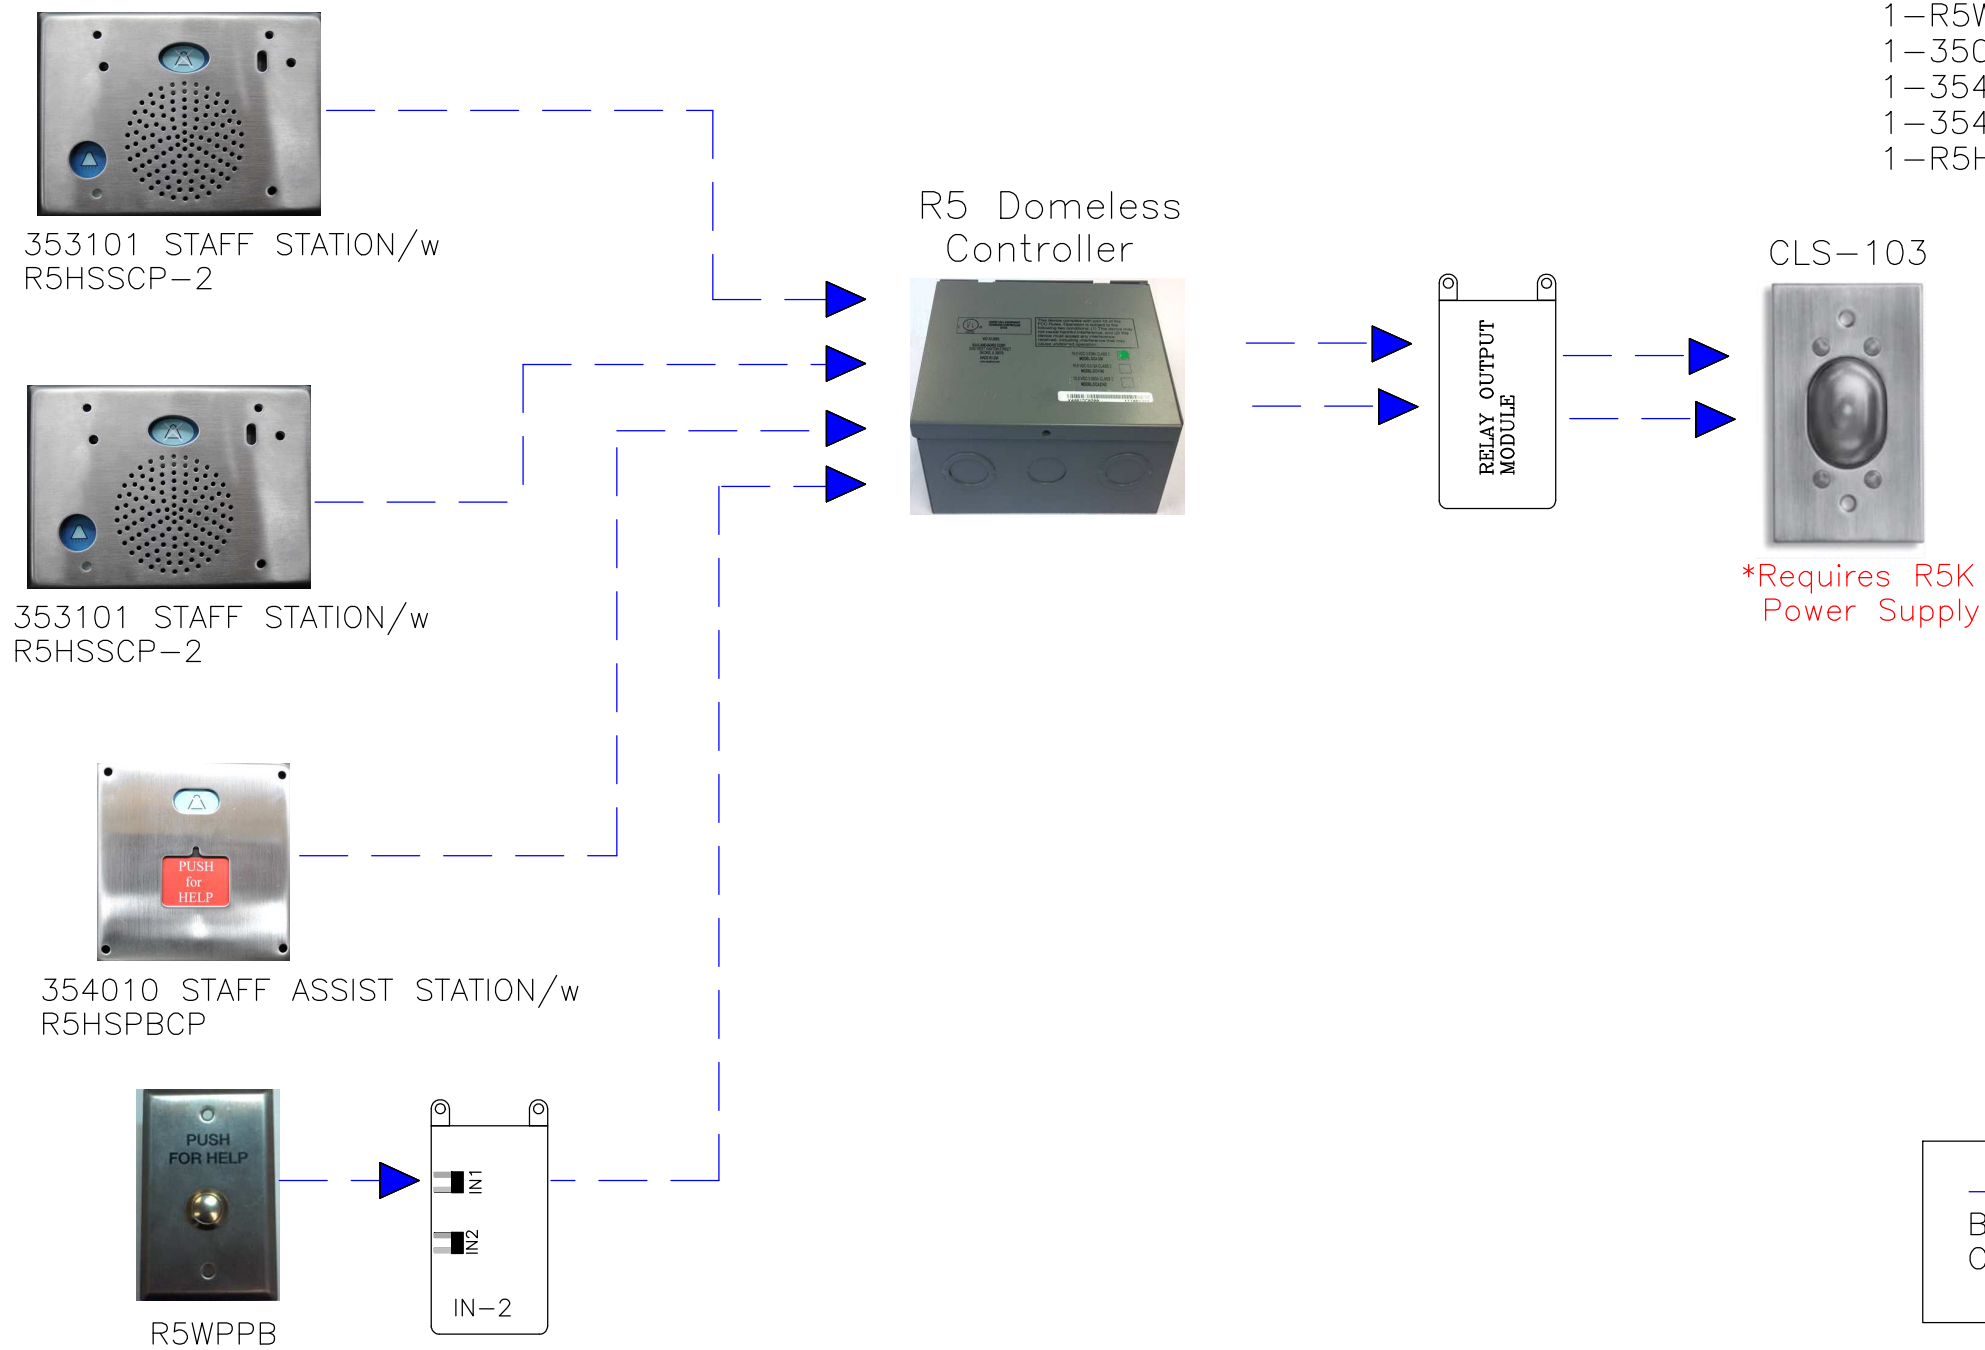

CALLS FROM R5WPPB CAN BE CANCELLED AT
STAFF STATION, PUSHBUTTON STATION OR CONSOLE

R5 High Security Key Lock Solution Option 3A

- Required Room Equipment:
- 2-353101 Staff Station
 - 2-R5HSSCP-1
 - 1-354010 Cancel Station
 - 1-R5HSCSCP
 - 1-352010 Dome Light
 - 3-354100-Input Module
 - 2-R5WPPB Water Resistant Call Switch
 - 2-350005 MNet Divider

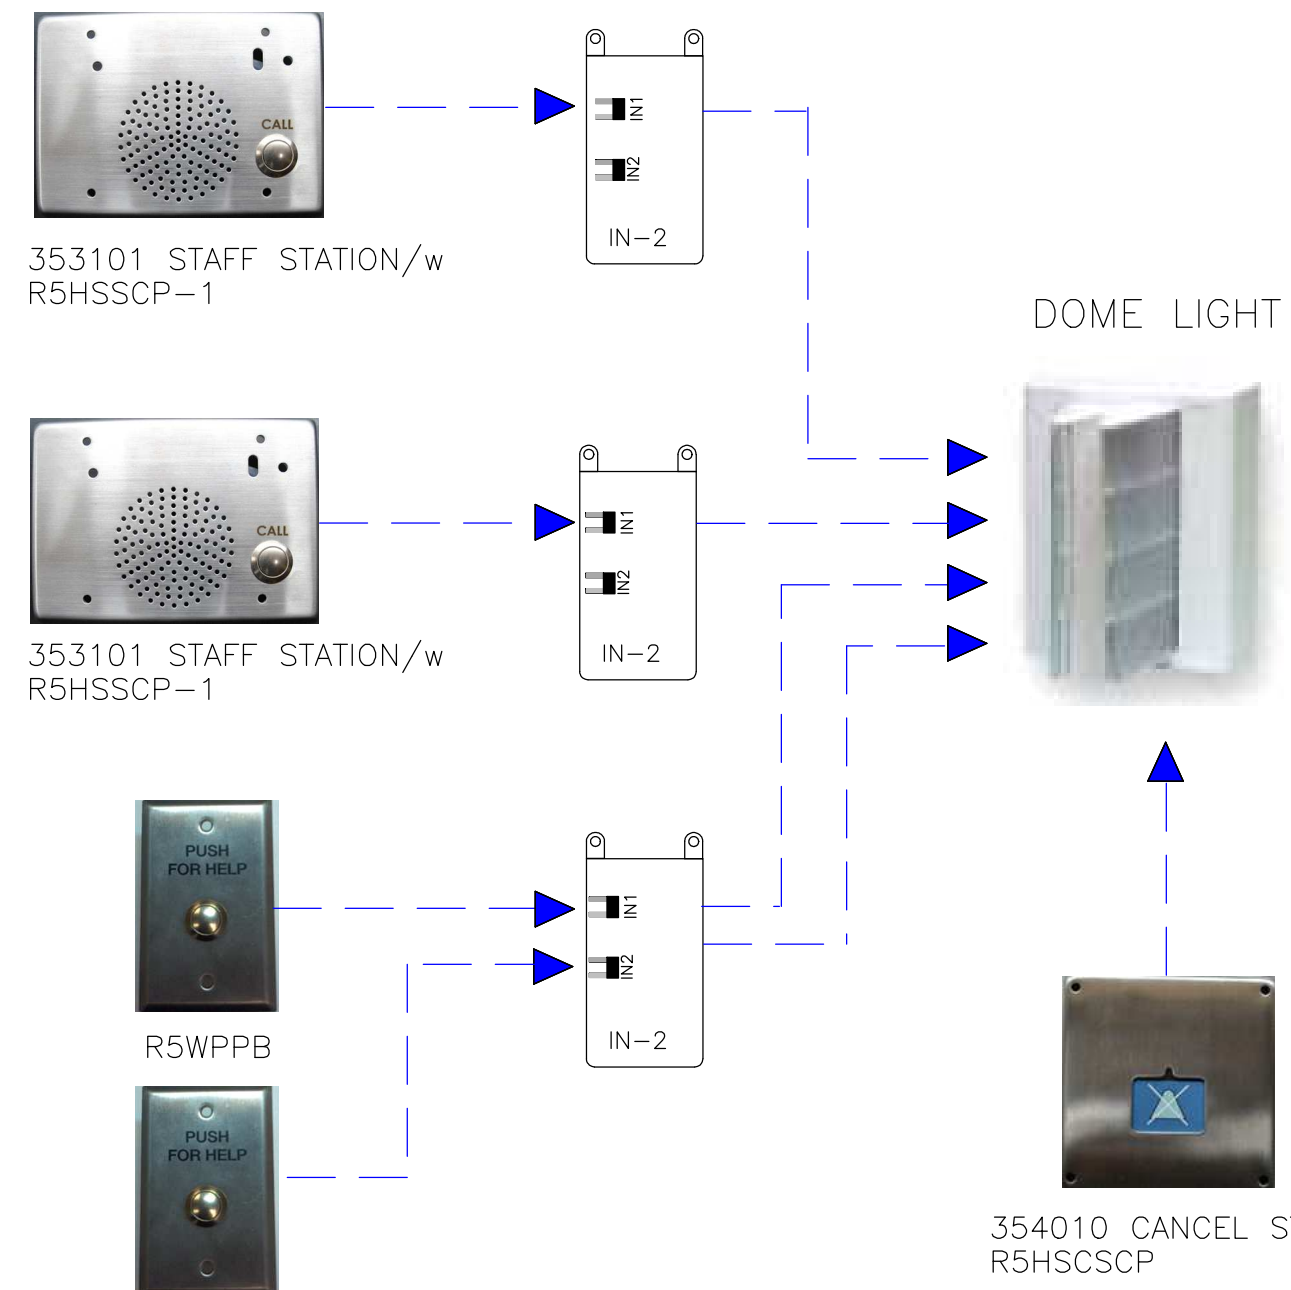


BLUE LINE REPRESENTS
CALL PATHWAY

ALL CALLS CAN BE CANCELLED AT
CANCEL STATION OR CONSOLE

R5 High Security Key Lock Solution Option 4

Required Room Equipment:

- 2-353101 Staff Station
- 2-R5HSSCP-1
- 1-354010 Cancel Station
- 1-R5HSCSCP
- 1-352021 Domeless Controller
- 3-354100- Input Module
- 1-354102 Relay Output Module
- 2-R5WPPB Water Resistant Call Switch
- 2-350005 MNet Divider
- 1-CLS-103 Dome Light

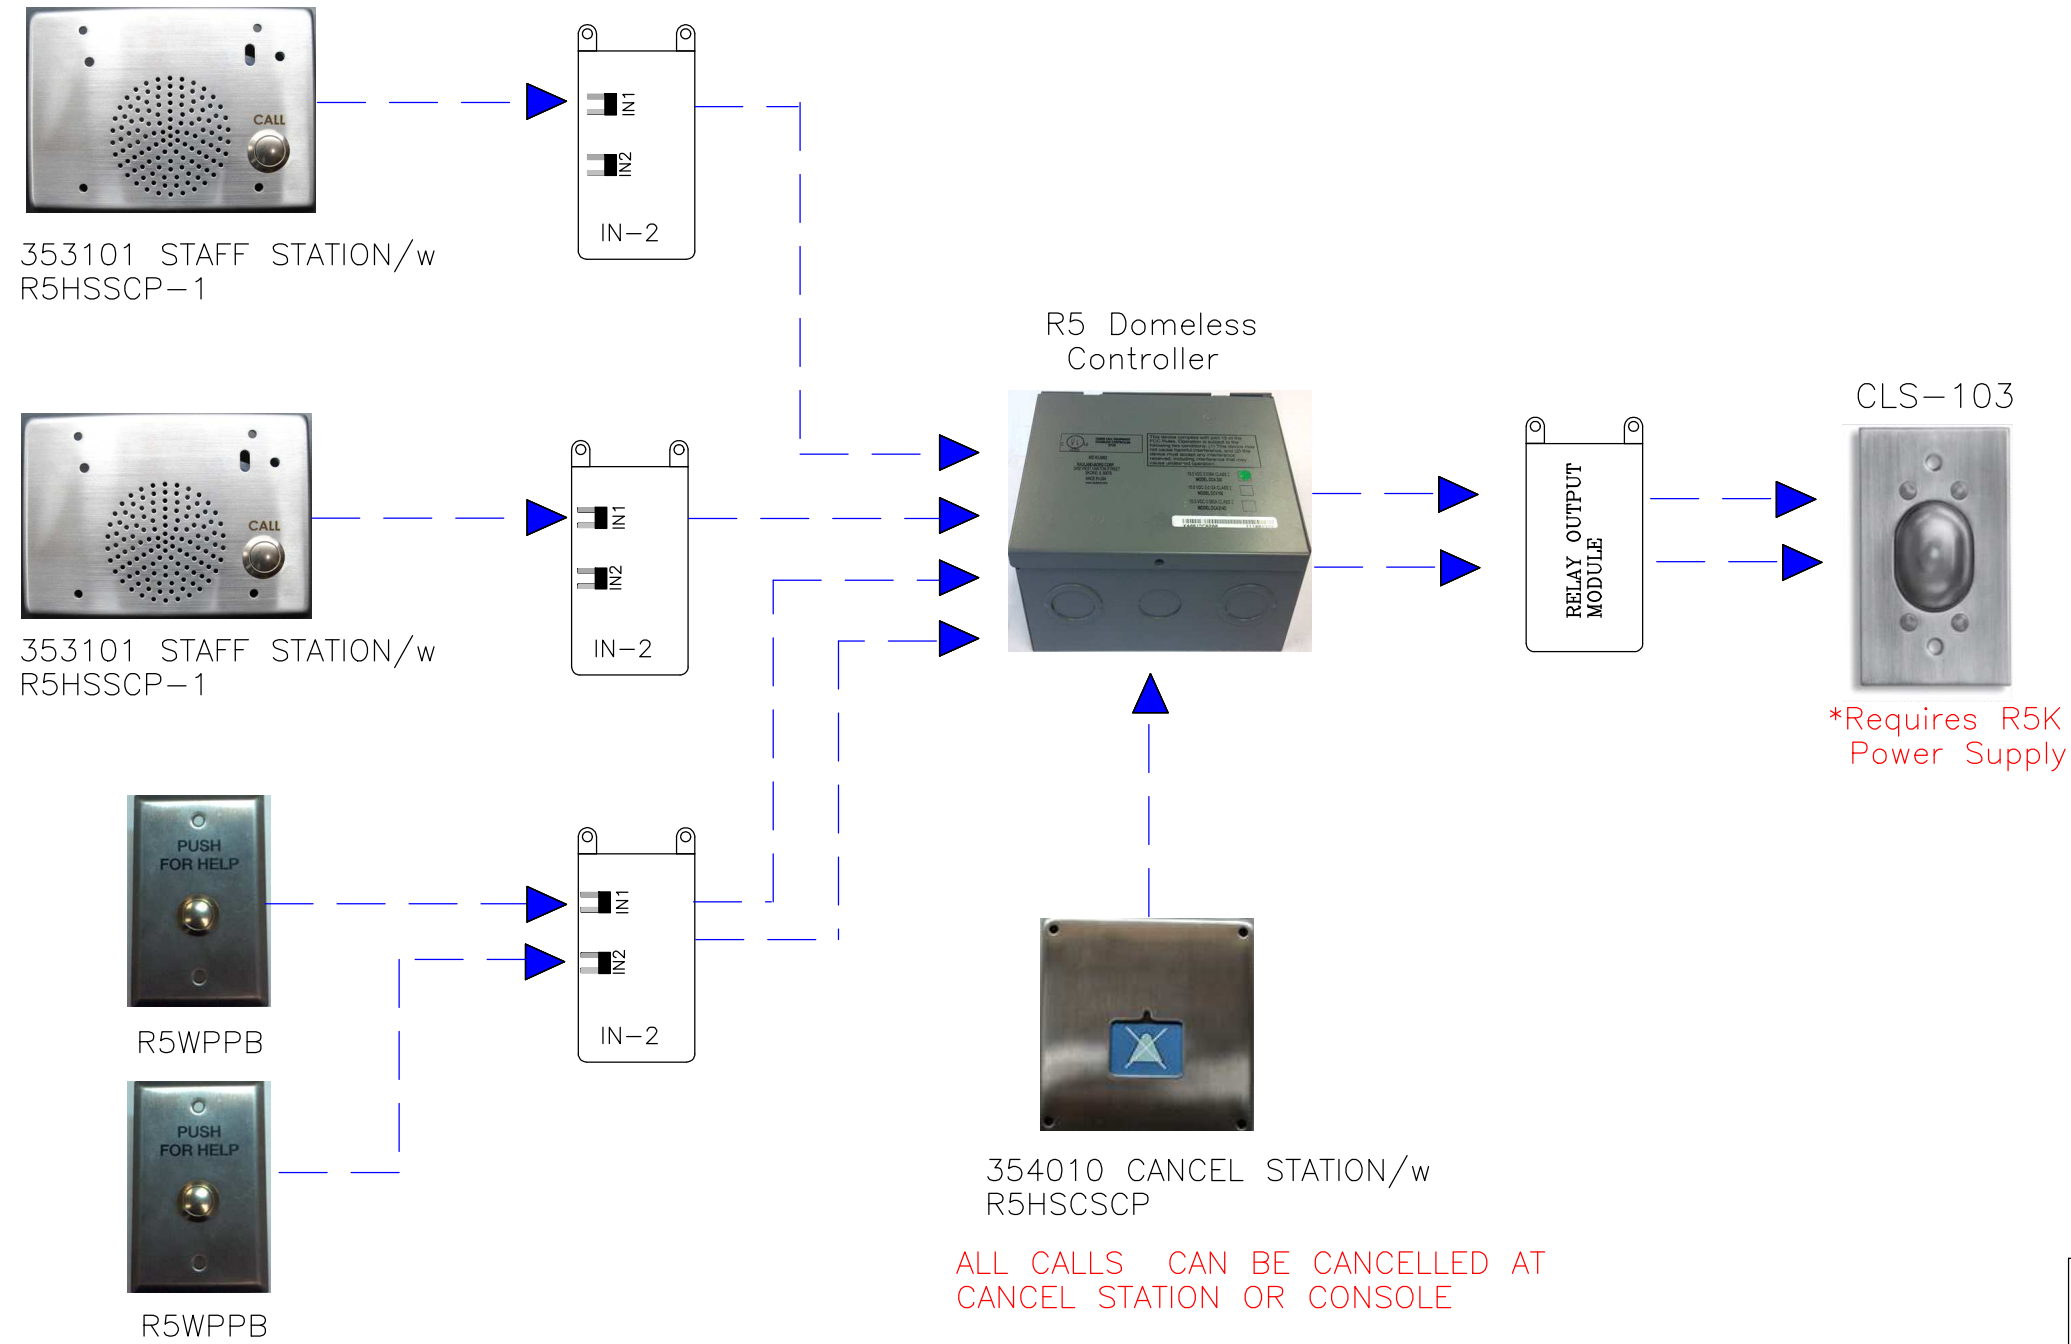

BLUE LINE REPRESENTS
CALL PATHWAY

R5 High Security Key Lock Solution Option 4A